


Stoma Platform

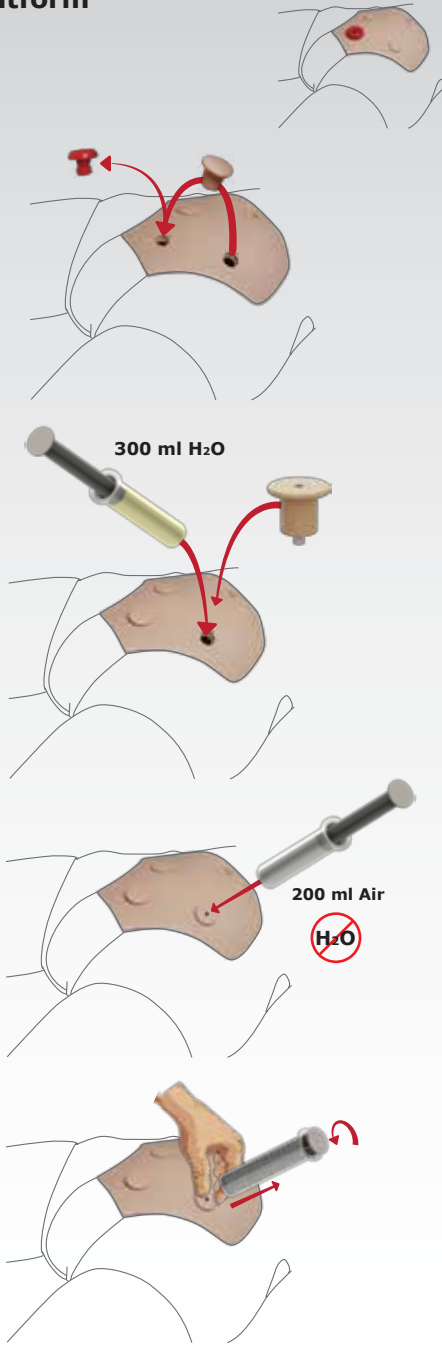

Ready for Simulation

Cleaning and Care:


Use only **isopropyl alcohol** on all parts.

Storage:

Dry all items before storing. One teaspoon of isopropyl alcohol may be added to the bladder to prevent mold growth.



Plug with Valve
(To Pressurize)

 Do not insert needles or sharp objects inside plug.



Solid Plug



Plug with Vent

Copyright 2012
Printed in USA
PN 20-05594 Rev A








Laerdal
helping save lives





Setup Guide Urinary Catheterization



Laerdal
helping save lives

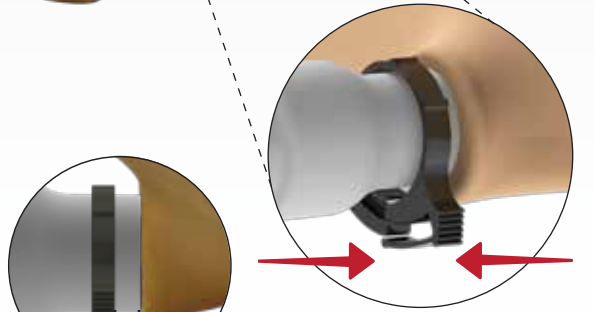
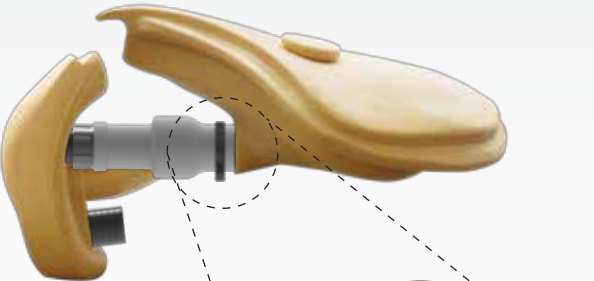
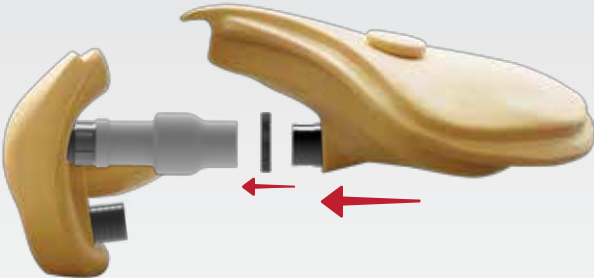
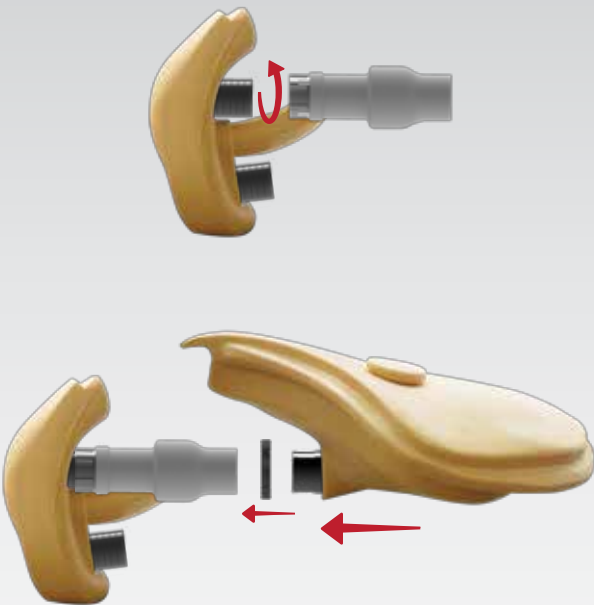


Male/Female Nursing Platform

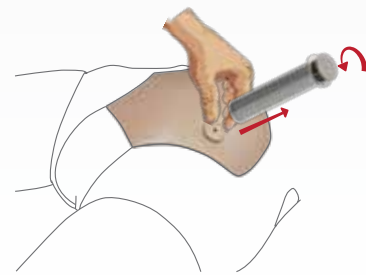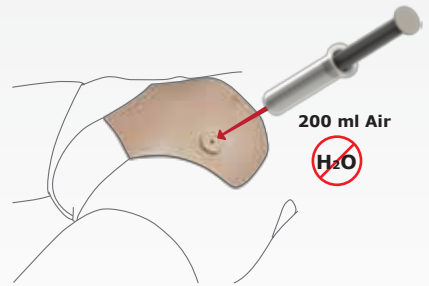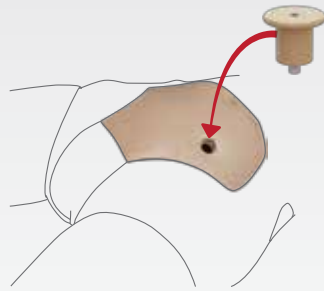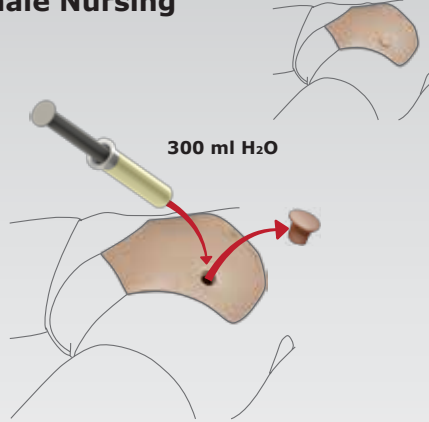

Ready for Simulation

ALS/MC Kelly Platform

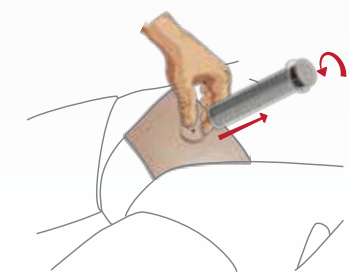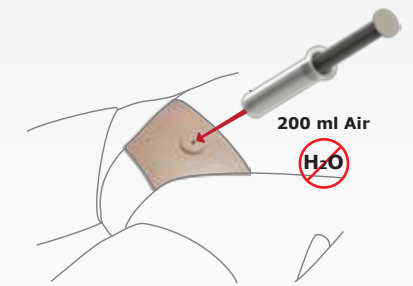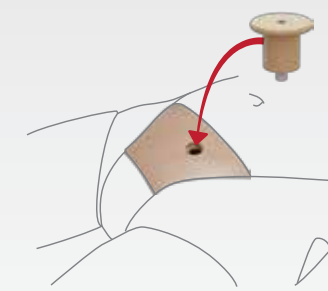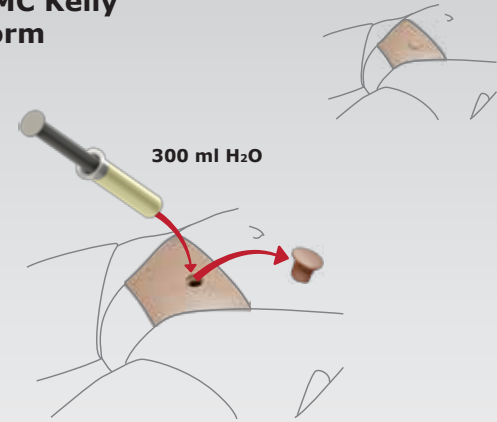

Ready for Simulation